

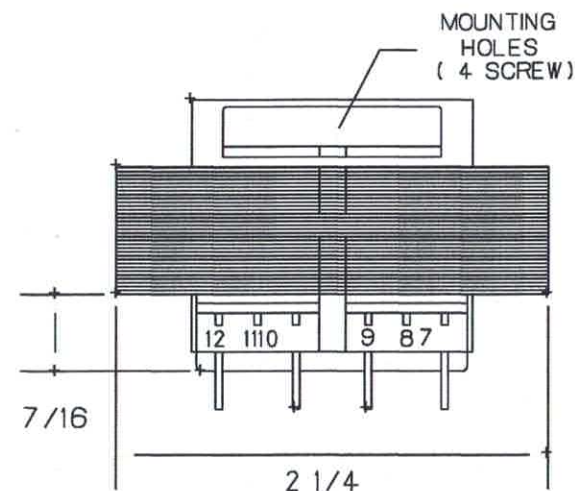


| REVISIONS |                           |        |          |
|-----------|---------------------------|--------|----------|
| LETTER    | DESCRIPTION               | DWG BY | DATE     |
| A         | ADDED NOTES               | SMS    | 8-20-14  |
| B         | REDRAWN AND UPDATED NOTES | SMS    | 1-20-17  |
| C         | PIN IDENTIFICATION        | JOW3   | 10-20-25 |

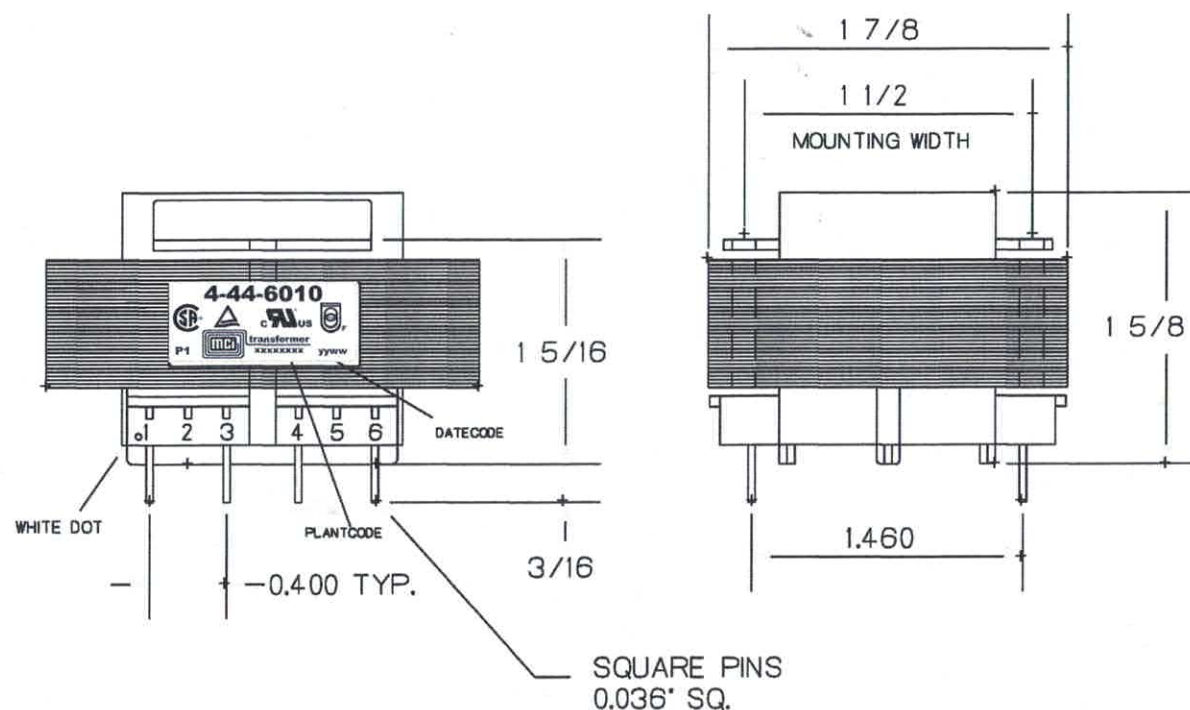

## NOTES:

- 1) UL INSULATION SYSTEM E86543-CLASS F 155°C.
- 2) UL RECOGNIZED COMPONENT: FILE #E86403
- 3) ISOLATION TRANSFORMER CONSTRUCTION UL 60601-1 AND CSA C22.2 NO. 601.1-M90: FILE #178395
- 4) TUV CERTIFIED: EN61558-1 AND EN61558-2-6, "IPOO: FAIL-SAFE SAFETY ISOLATION TRANSFORMER."
- 5) CSA CERTIFIED: FILE #LR80864
- 6) 4000 VRMS HIPOT BETWEEN PRIMARY AND (SECONDARY + CORE).  
500 VOLTS BETWEEN SECONDARY AND CORE.
- 7) WEIGHT: 0.90 LBS.
- 8) RoHS AND REACH COMPLIANT
- 9) ALL DIMENSIONS ARE IN INCHES.

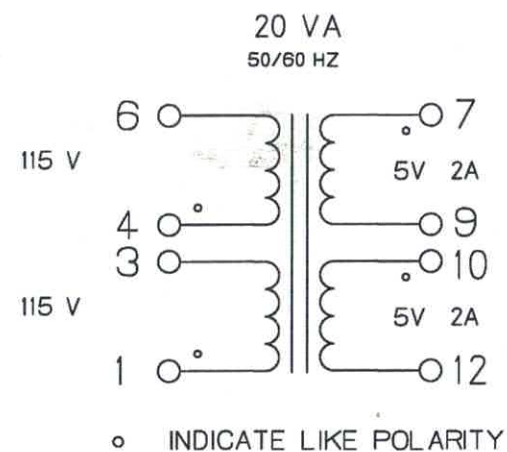

|                                    |            |       |        |                    |  |
|------------------------------------|------------|-------|--------|--------------------|--|
| MCI                                |            |       |        | NORTH BABYLON N.Y. |  |
| CUSTOMER                           |            |       |        |                    |  |
| MCI                                |            |       |        |                    |  |
| TITLE                              |            |       |        |                    |  |
| INTERNATIONAL STYLE PC TRANSFORMER |            |       |        |                    |  |
| DRAWN BY                           | APPROVD BY | SCALE | DATE   | DRAWING NUMBER     |  |
| SMS                                | JOW        | NONE  | 6-6-12 | 4-44-6010          |  |