



REVISIONS

LETTER	DESCRIPTION	DWG BY	DATE
A	ADDED NOTES	SMS	8-20-14
B	REDRAWN AND UPDATED NOTES	SMS	1-20-17
C	PIN IDENTIFICATION	JOW3	10-20-25

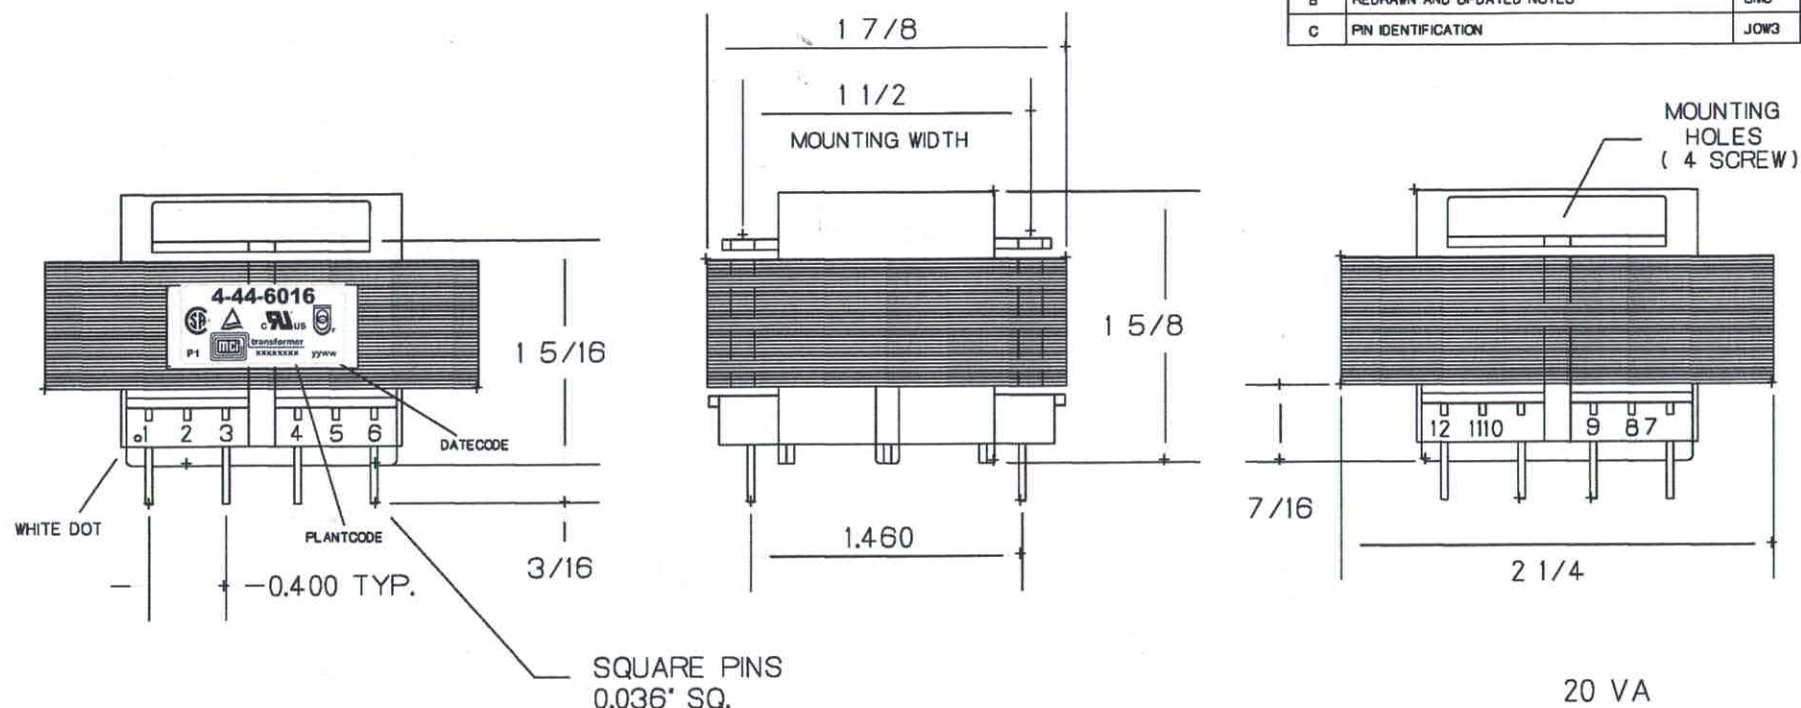

NOTES:

- 1) UL INSULATION SYSTEM E86543-CLASS F 155°C.
- 2) UL RECOGNIZED COMPONENT: FILE # E86403
- 3) ISOLATION TRANSFORMER CONSTRUCTION UL 60601-1 AND CSA C22.2 NO. 601.1-M90: FILE# 178395
- 4) TUV CERTIFIED: EN61558-1 AND EN61558-2-6, "IPOO: FAIL-SAFE SAFETY ISOLATION TRANSFORMER"
- 5) CSA CERTIFIED: FILE #LR80864
- 6) 4000 VRMS HIPOT BETWEEN PRIMARY AND (SECONDARY + CORE).
- 7) 500 VOLTS BETWEEN SECONDARY AND CORE.
- 8) WEIGHT: 0.90 LBS.
- 9) RoHS AND REACH COMPLIANT
- 9) ALL DIMENSIONS ARE IN INCHES.

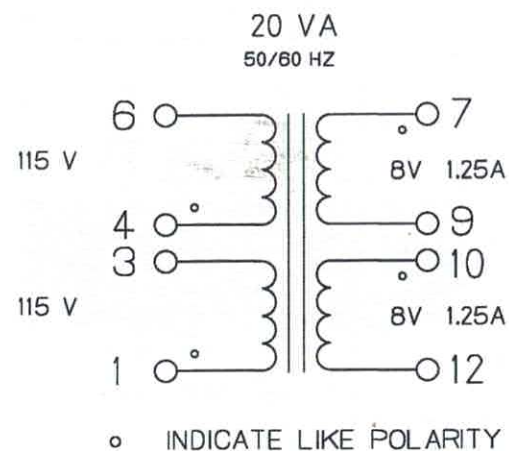

MCI				NORTH BABYLON N.Y.	
CUSTOMER					
MCI					
TITLE					
INTERNATIONAL STYLE PC TRANSFORMER					
DRAWN BY		APPRVD BY		DRAWING NUMBER	
SMS		JOW		4-44-6016	
SCALE		DATE			
NONE		6-6-12			