

## REVISIONS

| LETTER | DESCRIPTION | DWG BY | DATE |
|---|---|---|---|
| A | ADDED NOTES | SMS | 8-20-14 |
| B | REDRAWN AND UPDATED NOTES | SMS | 1-20-17 |
| C | PIN IDENTIFICATION | JOW3 | 10-20-25 |

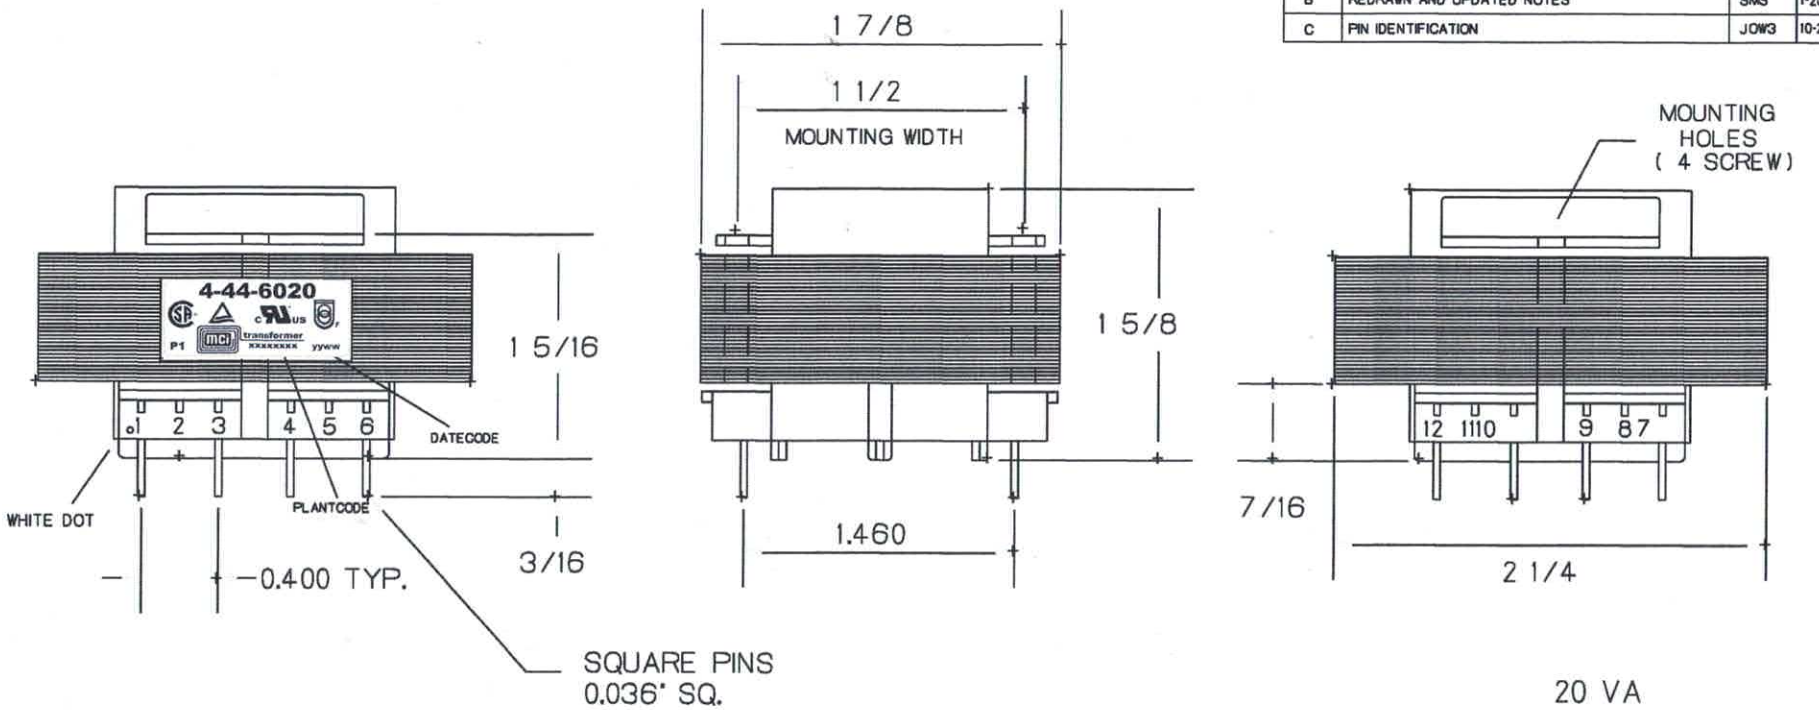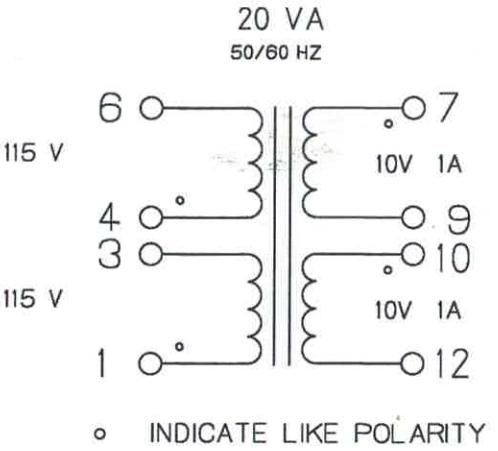


## NOTES:

1) UL INSULATION SYSTEM E86543-CLASS F 155°C.
2) UL RECOGNIZED COMPONENT: FILE # E86403
3) ISOLATION TRANSFORMER CONSTRUCTION UL 60601-1 AND CSA C22.2 NO. 601.1-M90: FILE #178395
4) TUV CERTIFIED: EN61558-1 AND EN61558-2-6, "IP00: FAIL-SAFE SAFETY ISOLATION TRANSFORMER ⓔ"
5) CSA CERTIFIED: FILE # LR80864
6) 4000 VRMS HIPOT BETWEEN PRIMARY AND (SECONDARY + CORE).
   500 VOLTS BETWEEN SECONDARY AND CORE.
7) WEIGHT: 0.90 LBS.
8) RoHS AND REACH COMPLIANT
9) ALL DIMENSIONS ARE IN INCHES.

MCI — NORTH BABYLON N.Y.

| CUSTOMER | | | | |
|---|---|---|---|---|
| MCI | | | | |
| TITLE | | | | |
| INTERNATIONAL STYLE PC TRANSFORMER | | | | |
| DRAWN BY | APPRVD BY | SCALE | DATE | DRAWING NUMBER |
| SMS | JOW | NONE | 6-6-12 | 4-44-6020 |